

Certificate of Analysis

Reformatted from image-based laboratory certificate for internal reference.
Original source image included below for evidentiary continuity.

COMPOUND Content 11.53 mg 98.968	BATCH / LOT Pending Review	SAMPLE ID integrity
LABEL CLAIM 10mg	RECEIVED Pending Review	TESTED 12/08/2025


Analytical Results

Test	Result	Unit	Spec	Method	Status
Purity	98.968%	%	As reported	HPLC-UV-MS	PASS
Content	10mg		10mg	HPLC-UV-MS	PASS
Identity	BPC		Match	MS/HPLC-MS	PASS

Source Attribution

Detected source style: generic
Original lab name: N/A
Analyst: N/A

Original Source Image

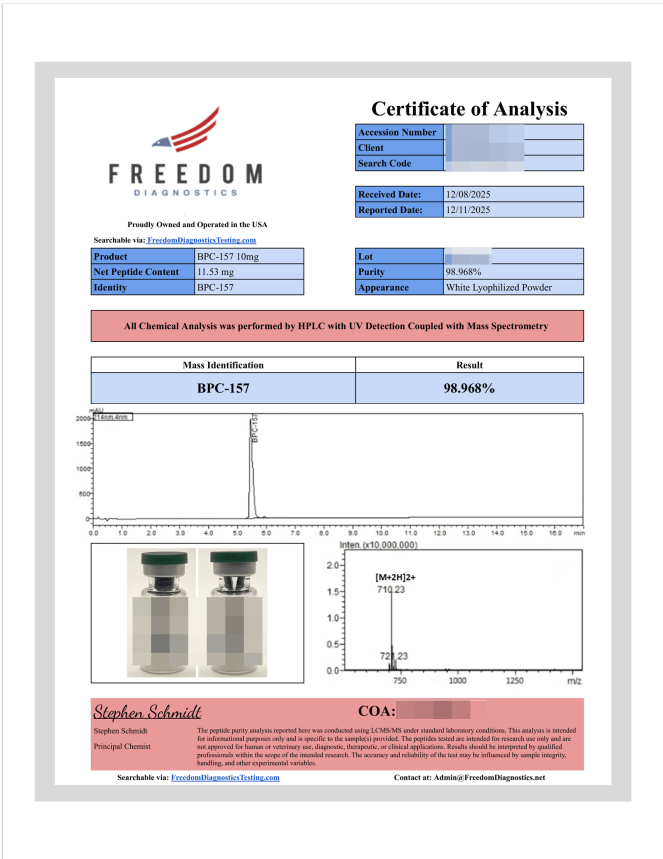

OCR Notes

Certificate of Analysis
TRUELABS.ME | health@truelabs.me | +61 481 835 854 (WhatsApp)

FB

SPO POT va TE DOP OOOO

Authorized Signatory

Laboratory Director
Research Use Only