

Certificate of Analysis

Reformatted from image-based laboratory certificate for internal reference.
Original source image included below for evidentiary continuity.

COMPOUND Content	BATCH / LOT Net	SAMPLE ID integrity
LABEL CLAIM 1000mg	RECEIVED Pending Review	TESTED 12/08/2025


Analytical Results

Test	Result	Unit	Spec	Method	Status
Purity	99.852%	%	As reported	HPLC-UV-MS	PASS
Content	1000mg		1000mg	HPLC-UV-MS	PASS
Identity	NAD		Match	MS/HPLC-MS	PASS

Source Attribution

Detected source style: generic
Original lab name: N/A
Analyst: N/A

Original Source Image

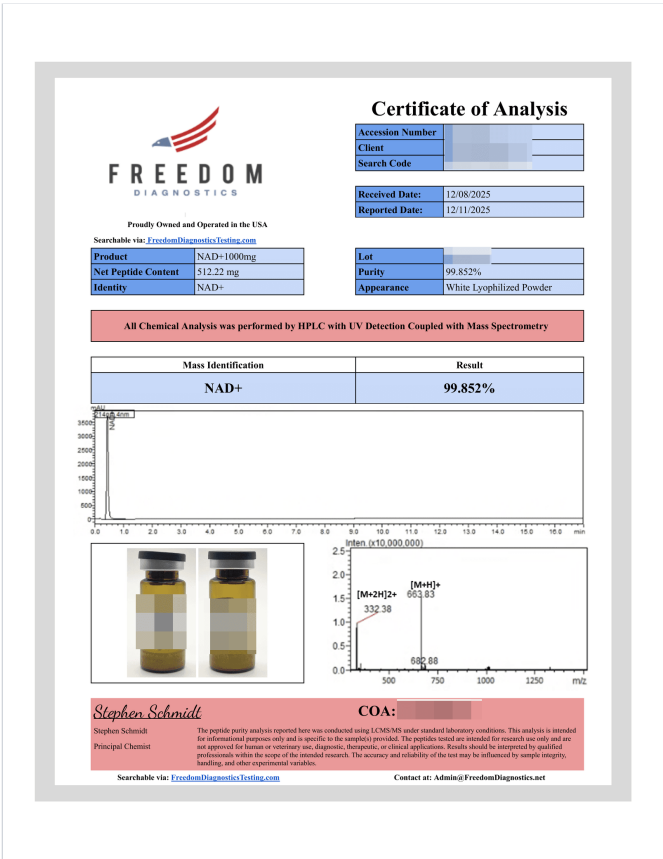

[Handwritten Signature]

OCR Notes

Certificate of Analysis
TRUELABS.ME | health@truelabs.me | +61 481 835 854 (WhatsApp)

ZA

ac

Authorized Signatory

Laboratory Director
Research Use Only